

Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with patent application GB0107708.0 filed on 28 March 2001.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.


In accordance with the rules, the words "public limited company" may be replaced by p.l.c., P.L.C. or PLC.

Registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

Signed



Dated 25 September 2007

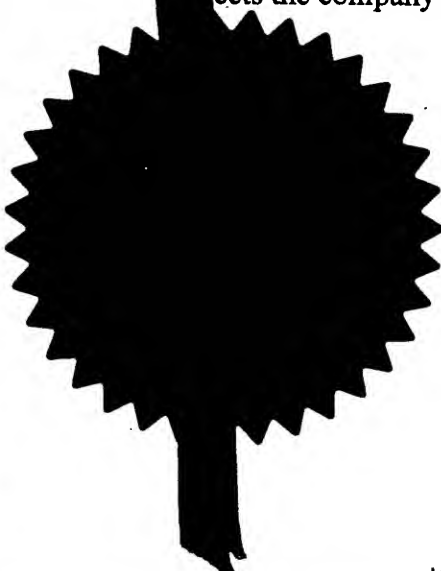



The
Patent
Office

1/77

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

1. Your reference	ICOU / P23522GB			28 MAR 2001
2. Patent application number (The Patent Office will fill in this)	0107708.0			28MAR01 E617512-9 D02866
3. Full name, address and postcode of the or of each applicant (underline all surnames)	Imperial College Innovations Ltd 47 Prince's Gate Exhibition Road London SW7 2QA United Kingdom			P01,7700 0.00 0107708.0 0107708.0
Patents ADP number (if you know it)				
If the applicant is a corporate body, give the country/state of its incorporation	United Kingdom			7409436001
4. Title of the invention	BONE FIXATED, ARTICULATED JOINT LOAD CONTROL DEVICE			
5. Name of your agent (if you have one)	ERIC POTTER CLARKSON PARK VIEW HOUSE 58 THE ROPEWALK NOTTINGHAM NG1 5DD			
"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)				
Patents ADP number (if you know it)	1305010			
6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number	Country	Priority application number (if you know it)	Date of filing (day / month / year)	
7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application	Number of earlier application		Date of filing (day / month / year)	
8. Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if:	YES			
a) any applicant named in part 3 is not an inventor; or				
b) there is an inventor who is not named as an applicant, or				
c) any named applicant is a corporate body.				
See note (d))				

Patents Form 1/77


9. Enter the number of sheets for any of the following items you are filing with this form.
Do not count copies of the same document

Continuation sheets of this form

Description 15

Claims(s) 6

Abstract 1

Drawing(s) 7 + 7 

-
10. If you are also filing in any of the following, state how many against each item.

Priority Documents 0

Translations of priority documents 0


Statement of inventorship and right to grant of a patent (*Patents Form 7/77*) YES

Request for preliminary examination and search (*Patents Form 9/77*) NO

Request for substantive examination (*Patents Form 10/77*) NO

Any other documents
(please specify)

-
11. I/We request the grant of a patent on the basis of this application.



Signature
ERIC POTTER CLARKSON

Date
27 March 2001


-
12. Name and daytime telephone number of person to contact in the United Kingdom 0115 9552211
-

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 01645 500505.
- Write your answers in capital letters using black ink or you may type them.
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- Once you have filled in the form you must remember to sign and date it.
- For details of the fee and ways to pay please contact the Patent Office.

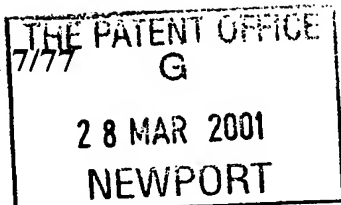

Statement of inventorship and of right to grant of a patent

1. Your reference	ICOU / P23522GB							
2. Patent application number (if you know it)	0107708.0	28 MAR 2001						
3. Full name of the or of each applicant	Imperial College Innovations, Ltd							
4. Title of the invention	BONE FIXATED, ARTICULATED JOINT LOAD CONTROL DEVICE							
5. State how the applicant(s) derived the right from the inventor(s) to be granted a patent	By Assignment							
6. How many, if any, additional Patents Forms 7/77 are attached to this form? (see note (c))								
7.	<p>I/We believe that the person(s) named over the page (and on any extra copies of this form) is/are the inventor(s) of the invention which the above patent application relates to.</p> <table border="0" style="width: 100%;"> <tr> <td style="width: 60%;">Signature</td> <td style="width: 40%;">Date</td> </tr> <tr> <td style="text-align: center;"><i>Eric Potter Clarkson</i></td> <td></td> </tr> <tr> <td style="text-align: center;">ERIC POTTER CLARKSON</td> <td style="text-align: center;">27 March 2001</td> </tr> </table>		Signature	Date	<i>Eric Potter Clarkson</i>		ERIC POTTER CLARKSON	27 March 2001
Signature	Date							
<i>Eric Potter Clarkson</i>								
ERIC POTTER CLARKSON	27 March 2001							
8. Name and daytime telephone number of person to contact in the United Kingdom	0115 9552211							

Notes

- a) If you need help to fill in this form or you have any questions, please contact the Patent Office on 01645 500505.
- b) Write your answers in capital letters using black ink or you may type them.
- c) If there are more than three inventors, please write the names and addresses of the other inventors on the back of another Patents Form 7/77 and attach it to this form.
- d) When an application does not declare any priority, or declares priority from an earlier UK application, you must provide enough copies of this form so that the Patent Office can send one to each inventor who is not an applicant.
- e) Once you have filled in the form you must remember to sign and date it.

Enter the full names, addresses and postcodes of the inventors in the boxes and underline the surnames

Edward Draper

771 London Road
Loudwater
Buckinghamshire
HP11 1HW
United Kingdom

Patents ADP number (if you know it):

8113920001

Patents ADP number (if you know it):

Patents ADP number (if you know it):

Reminder

Have you signed this form?

BONE FIXATED, ARTICULATED JOINT LOAD CONTROL DEVICE

5 The present invention relates to devices for restricting or controlling the movement or loading levels on joints in the human or animal body.

10 The human or animal body uses articular cartilage to surface many of its joints. This tissue tolerates relatively high levels of compression while having a low coefficient of friction – approximately that of wet ice on wet ice.

15 Bone, on which the cartilage is supported, is stiffer and stronger. Away from the joints, bone normally forms in large, thick-walled tubes. However, under the cartilage at the joints, the bone forms a three dimensional mesh of so called "cancellous" bone. Cancellous bone is more compliant than the rest of the bone structure and helps spread the load that the cartilage experiences, thus reducing the peak stresses on the cartilage.

20 Both cartilage and bone are living tissues that respond and adapt to the loads they experience. There is strong evidence that the loads that joint surfaces experience can be categorised into four regions or "loading zones".

1. *Under-loading zone.*

25 If a joint surface remains unloaded for appreciable periods of time the cartilage tends to soften and weaken.

2. *Healthy zone.*

30 Joint surfaces can and do last a lifetime and if they experience healthy levels of load they can be considered to effectively last indefinitely.

3. *Tolerant zone.*

As with engineering materials that experience structural loads, both bone and cartilage begin to show signs of failure at loads that are below their ultimate strength. Unlike engineering materials, however, cartilage and bone have some ability to repair themselves, bone more so. There are levels of loading that will cause micro-structural problems and trigger the repair processes. The body can tolerate these load levels as long as it has time to recuperate.

10 4. *Overloaded zone.*

There comes a level of load at which the skeleton will fail catastrophically. If the load level on a joint surface reaches this level even once then there will be severe consequences.

15 One of the major consequences of excessive loading is osteoarthritis. This loading could be either from a single overload in the overloaded zone or from loading within the tolerant zone too frequently.

20 The picture of safe joint loading is further complicated by the cascade of events that occur during the onset of osteoarthritis. These events include the break up of the cartilage, and bone 'sclerosis' in which the bone becomes denser and stiffer. This means that the maximum level of loading that can be considered healthy or tolerated falls, almost certainly to levels below that experienced in walking and standing.

25

Newly implanted grafts or tissue-engineered constructs will also have lower tolerance limits while they are establishing themselves within the joint.

In fact the treatment of osteoarthritis and other conditions is severely hampered when a surgeon is not able to control and prescribe the levels of

joint load. Furthermore, bone healing research has shown that some mechanical stimulation can enhance the healing response and it is likely that the optimum regime for a cartilage/bone graft or construct will involve different levels of load over time, eg. during a particular treatment schedule.

5

There is a need for a device that will facilitate the control of load on a joint undergoing treatment or therapy, to enable use of the joint within the healthy loading zone, or even within the healthy and tolerant loading zones, during the treatment episode.

10

There is further need for a device to preferably provide such control while allowing full, or relatively full mobility of a patient undergoing the treatment.

15

Such devices would be desirable particularly during the early treatment of, for example, an osteoarthritic joint. Under an appropriate treatment regime providing controlled loading, the condition of the joint may improve, possibly back to full health.

20

In the prior art, existing load controlling regimes and devices for use in treatment or therapy of articulating joints include the following.

a) Bed-rest or isolation of a joint is possible but, as indicated above, the long-term consequences of applying no load or generally maintaining the joint in the underloaded zone are not good.

25

b) Passive movement of a joint has been tried with some success. During this treatment, movement is applied to the joint by an external device while the joint is rested. However, this does not give the opportunity to vary

the load levels on the joint, eg. to work the joint within the healthy zone for that joint at any given stage of the treatment program.

5 c) Traction across a joint has long been used to counteract the compressive loads normally experienced by the joint. This is done either in bed or using an external fixator. Fixators exist which not only apply traction, but also have simple hinges to allow some joint motion.

10 d) External braces have been used to apply a bending moment across the joint and at 90° to the motion to move the centre of pressure from one part of the joint to another. However, since these braces are not attached directly to the skeleton, control of the applied loads is poor.

15 According to one aspect, the present invention provides an apparatus for controlling the load on articular cartilage of a human or animal joint comprising:

a first fixation assembly for attachment to a first bone;
a second fixation assembly for attachment to a second bone; and
a link assembly coupled to the first fixation assembly by a first pivot
20 and coupled to the second fixation assembly by a second pivot,
the first and second fixation assembly thereby each being angularly displaceable relative to the link assembly.

25 According to another aspect, the present invention provides a method of controlling loading on a joint comprising the steps of:

attaching a first fixation assembly to a first bone;
attaching a second fixation assembly to a second bone, the second bone being connected to the second bone by an articulating joint;
coupling said first fixation assembly and said second fixation
30 assembly by way of a link assembly so that said first fixation assembly and

said second fixation assembly are each angularly displaceable relative to the link assembly.

Embodiments of the present invention will now be described by way of
5 example and with reference to the accompanying drawings in which:

Figure 1 shows a perspective view of a fixator for controlling loads on articular cartilage according to a preferred embodiment of the present invention;

Figure 2 shows a perspective view of a pair of fixators of figure 2 in a
10 dual sided or bilateral configuration;

Figure 3 shows perspective views of a selection of central modules suitable for use with the fixators of figures 1 and 2;

Figure 4 shows a perspective view of an externally powered fixator;

Figure 5 shows perspective views of a selection of alternative fixation
15 assemblies suitable for use in the fixators of figures 1 and 2;

Figure 6 shows a plan view of a bilateral configuration of fixators as in figure 2, illustrating the effects of unilateral variation in the length of link assembly; and

Figure 7 shows a parallel-crosswise configuration of link assembly.
20

With reference to figure 1, there is shown an articulated joint load controlling device or fixator 10 according to one embodiment of the invention. The fixator 10 comprises a first fixation assembly 11, a second fixation assembly 12 and a link assembly 13 connecting the first and second
25 fixation assemblies 11, 12.

The first and second fixation assemblies 11, 12 are each coupled to the link assembly 13 by a pivot 14, 15 or other equivalent means facilitating angular displacement of the respective fixation assembly to the link assembly.
30 Throughout the present specification, use of the word "pivot" is intended to

encompass all such equivalent means for facilitating angular displacement. It will be understood that the first and second fixation assemblies 11, 12 are therefore not only angularly displaceable relative to one another, but are also capable of some relative translational movement subject to the geometric
5 limitations provided by the link assembly 13.

Preferably, the axes of the pivots 14, 15 are parallel so that the first and second fixation assemblies 11, 12 will rotate about the link assembly in the same plane.

10 In an alternative embodiment, however, the pivots 14 and 15 might not be axially parallel, in order to better follow the three-dimensional movement of a particular joint. In a further embodiment, one or both pivots 14, 15 might be of the universal joint type, such that the pivot allows two degrees of
15 rotational freedom rather than only a single degree of rotational freedom, in order to better follow the three-dimensional movement of, for example, a ball joint.

Each fixation assembly 11, 12 preferably comprises a faceplate 20 having
20 one or more slots 21 defined in the faceplate surface. Coupled to the faceplate 20 is a clamp plate 22 which may be tightened onto the faceplate 20 by way of screws, or other means known in the art. Preferably, the clamp plate includes corresponding slots 23. As shown more clearly in figure 2, the face plate 20 and clamp plate 22 together provide an anchorage for one or
25 more bone pins 30 which can be screwed into or otherwise fixed to a bone using known techniques. Other examples of fixation assemblies are illustrated later in connection with figure 5.

In the arrangement of figure 1, a single load controlling fixator 10 may be
30 attached to an articulating joint by way of first bone pins 30 screwed into

one side of a first bone using the first fixation assembly 11, and second bone pins 30 screwed into a corresponding side of a second bone using the second fixation assembly 12. The first and second bones are on either side of an articulating joint to be controlled by the fixator.

5

In the arrangement of figure 2, two load controlling devices or fixators may be used in a bilateral configuration on either side of an articulating joint, the bone pins 30 passing right through the respective first and second bones on either side of the articulating joint. By applying compression in one fixator and tension in the other fixator, it is possible to apply a bending moment to the joint so as to move the centre of pressure within the joint in a controlled manner and so relieve the loads experienced by the areas of concern.

In further embodiments, first and second fixation assemblies 11, 12 of a fixator 10 might be coupled to two or more link assemblies in series or in parallel with one another. For example, as shown in figure 7, a fixator 16 comprises a first fixation assembly 11 and a second fixation assembly 12 that are connected by a link assembly that comprises a pair of link members 18, 19 in a parallel-crosswise configuration. Each link member is pivotally anchored to both the first and second fixation assemblies 11, 12 by way of face plates 17, the link members being laterally displaced from one another. In the embodiment shown, the link member 18 and link member 19 are not only laterally displaced from one another, but also angularly displaced from one another, in a crosswise formation. This arrangement provides a controlled, limited degree of freedom of relative movement of the first and second fixation assemblies. By adjusting the position of the two link members it is possible to mimic the movement of the knee.

Referring now to figure 3, various arrangements of link assemblies and their respective functions will now be described.

In a first arrangement, labelled figure 3A, the link assembly 40 comprises a rigid, fixed length member having a barrel centre section 41 and a pair of lugs 44 extending from each end. Each pair of lugs 44 includes a pair of coaxial apertures or hubs 42, 43 in which can rotate respective pivot pins 14, 15 (figure 1). Each pair of lugs 44 define therebetween a slot 45 adapted to receive a corresponding lug 25 (see figure 1) of a respective fixation assembly 11 or 12. The link assembly 40 essentially maintains first and second pivots 14 and 15 at a fixed distance of separation.

10

In a further embodiment, the lug pairs 44 and barrel centre section 41 may be screwed together for quick disassembly and re-assembly, enabling different length barrel centre sections 41 to readily be used to provide a link assembly 40 of an appropriate length to the joint under treatment or therapy and to be changed during a treatment program.

15

In another arrangement, labelled figure 3C, a link assembly 50 provides for a variable distance of separation of pivots 14, 15 in hubs 52, 53. Link assembly 50 comprises a pair of lugs 54 and a pair of lugs 55, each pair being mounted on a central shaft 56 and being axially displaceable therealong. A pair of tension springs 57, 58 provide a means for biasing the distance of separation of the pivots 14, 15 towards a minimum limit of separation of the lug pairs 54, 55 to apply greater compression forces than those normally experienced by the joint.

25

In another arrangement, labelled figure 3D, a link assembly 60 provides for a variable distance of separation of pivots 14, 15 in hubs 62, 63. Link assembly 60 comprises a pair of lugs 64 and a pair of lugs 65, each pair being mounted on a central shaft 66 and being axially displaceable therealong. A compression spring 67 provides a means for biasing the

30

distance of separation of the pivots 14, 15 towards a maximum limit of separation of the lug pairs 64, 65 so as to counteract the natural compressive forces experienced by the joint.

- 5 It will be understood that the functions of link assembly 50 and link assembly 60 may be combined to provide bias towards a central position so that there is resistance against movement of the pairs of lugs from a centre position. More generally, this provides means for biasing the first and second pivots towards an intermediate distance of separation between
10 predetermined limits of separation of the lug pairs 54, 55 or 64, 65.

- Although not shown in figures 3C or 3D, it is also possible to provide a locking member which is axially adjustable along the length of the link assembly to adjust the limit or limits of separation of the lug pairs. The
15 locking member could be provided, for example, by way of a screw-threaded collar on the central shaft 56 or 66 using techniques that will be understood by those skilled in the art.

- In another arrangement, labelled as figure 3F, the provision of a means for
20 controlling the distance of separation of pivots 14, 15 could be by way of a link assembly 80 that includes a pneumatic or hydraulic cylinder 81, controlled externally by a controller (not shown) connected thereto by two feed pipes 82, 83. The pneumatic or hydraulic cylinder may also provide means for biasing the distance of separation of the first and second pivots to
25 a predetermined position.

It will be understood that the functions of the pneumatic or hydraulic cylinder 81 could be alternatively provided by an electrically driven system.

In another arrangement, labelled figure 3E, the link assembly 70 (which may generally correspond with a links 50 or 60 having variable separation members) may also be provided with a mechanism for varying the distance of separation of the pivots 14, 15 according to the angular displacement of the first and/or second fixation assemblies relative to the link assembly. This would enable, for example, the separation to be increased in the last 5° of angular displacement.

In the preferred embodiment shown, a cam surface 76, 77 is provided on the circumferential edge of one or both of the lug pairs 74, 75. The cam surface bears on a corresponding bearing surface on a respective fixation assembly 11, 12 and is preferably adapted to vary the separation of the fixation assemblies as a function of the angular displacement. As an example, for a fixator attached to a knee joint, the cam surfaces 76, 77 can be arranged so that as the knee is moved to the fully extended condition, the fixator ensures a greater separation of the fixation assemblies 11, 12 thereby reducing pressure on the joint surfaces.

In another arrangement, the cam surfaces 76, 77 could be adapted to limit the angular displacement of that fixation assembly.

In another arrangement, the cam surfaces may be used to provide a varying degree of resistance to angular displacement of the fixation assembly. More generally, the cam surface may be adapted to provide a means for progressively increasing resistance to angular displacement of the fixation assembly relative to the link assembly as a function of the angular displacement from a reference position.

The means for limiting angular displacement could alternatively be provided by a stepped surface on the circumferential edge of the lug in a manner which will be understood by those skilled in the art.

- 5 In conjunction with any of the link assemblies described above, a link assembly 90 as shown in figure 3B may be provided with means for recording loads applied across the link assembly. The sensor may be adapted to monitor any one or more of the tensile load, the compression load, shear forces or bending forces applied across the link assembly.
- 10 Preferably the sensor comprises a strain gauge. Such a device makes it possible to determine the load actually being carried by a joint. In the preferred embodiment shown, this is achieved by the installation of strain gauges 92 into the barrel 93 of the link assembly 90.
- 15 Separate transducers could be added to monitor angular displacement of the fixation assemblies relative to the link assembly 90.

In another arrangement, as shown in figure 4, the angular displacement of the fixation assemblies relative to one another may be controlled externally.

- 20 This can be achieved by a linear actuator 100 linked to the first and second fixation assemblies 11, 12 by way of brackets 17, 18 each extending from a respective fixation assembly in a direction orthogonal to the pivot axis.

- The linear actuator 100 may be powered electrically, pneumatically or hydraulically and enables movement of a joint to be automatically controlled for exercise within the healthy load zone without use of the associated musculature.
- 25

- Referring back to figure 2, it will be noted that when the various link assemblies described in connection with figure 3 are used in the bilateral
- 30

- configuration, it is possible, by varying the length of the link assembly 13 independently on either side of the joint, to alter the position of the centre of pressure in the joint. This can be particularly useful in the treatment of knees. An example of the effects of this is illustrated in figure 6. In the figure, a bilateral configuration of fixation assemblies is shown similar to that of figure 2, viewed from above (ie. generally perpendicular to the pivot axes). In this example, fixation assemblies 11a, 12a and 11b, 12b are respectively connected by link assemblies 13a, 13b. A unilateral adjustment of the length of link assembly 13b results in a relative angular displacement of the bones 4, 5 that varies with articulation of the bones about the axis of the joint, thereby imposing an angulation on the joint. This will tend to have the effect of reducing the load experienced at the joint surface on the side nearest to the lengthened segment.
- 15 With reference to figure 5, alternative arrangements of fixation assemblies which themselves facilitate further angular degrees of freedom of the fixator are now described. Figure 5A shows a fixation assembly 110 have a lug 25 for attachment to the various possible link assemblies 13, 40, 50, 60, 70, 80, 90. The body of the fixation assembly includes a plurality of apertures 111a, 111b, 111c each adapted to receive a bone pin 30. In this arrangement, however, each aperture is defined in a corresponding rotatable collar 112a, 112b, 112c such that the angles of the bone pins 30 may be varied on and about the central longitudinal axis of the fixation assembly 110.
- 25 The fixation assembly 120 as shown in figure 5b is similar to that of figure 5a, except that in this case the apertures 121a, 121b, 121c are laterally offset from the central longitudinal axis of the fixation assembly. Each aperture is again defined in a corresponding rotatable collar 122a, 122b, 122c so that the angles of the bone pins 30 may be varied about a longitudinal axis that is

laterally displaced from the central longitudinal axis of the fixation assembly 120.

5 The fixation assembly 130 as shown in figure 5c provides a further degree of freedom. In this arrangement, bone pins 30 are located in slots 131 formed between a first clamp plate 132 and a second clamp plate 133. The clamp plates 132, 133 are rotatable about a first axis (transverse to a longitudinal axis of the fixation assembly 130) on pivot 134, and about a second axis (preferably a longitudinal axis of the fixation assembly 130) on pivot 135.
10 Taken together with the pivot through aperture 136, this provides a full three rotational degrees of freedom of the bone relative to a link assembly.

The fixator device embodiments as generally described above therefore provide a means for applying and/or limiting tension, compression, torsion,
15 bending and shear forces to an articulated joint in a controlled manner and provide for some or all of the following treatment regimes either in isolation or in any combination. Also it will be possible to change the regime or combination of regimes easily and without the need for a sterile environment or anaesthesia. It is noted that joints of the skeleton naturally experience
20 compression and the fixators of the present invention can provide amelioration of this by applying tension.

1. *Continuous traction.*

The level of tension can be varied according to the length of the link
25 assembly used and this can be further varied according to the bias strengths applied by the springs 57, 58, 67.

2. *Partial or full support.*

Some or all of the compression that would otherwise be carried by the joint may be taken by the device, and this can be a function of the angle of support by control of spring strength and angle of fixation to the bones.

5 3. *Application of a bending moment, torsion or shear force.*

Application of these loads to the joint allows the clinician to move the centre of pressure within the joint to regions that are healthy.

4. *Application of an externally powered loading regime.*

10 This can occur normally while the subject is at rest at set angles, load levels, loading and unloading rates and frequencies using the powered embodiments described above. Providing a portable power supply will, however, allow the patient to continue to move freely.

15 5. *Allowing the joint load to be gradually increased.*

This may be desirable at the end of a treatment episode. This can be done either by applying additional compression or a bending moment, shear force or torsion in the opposite direction from that described above.

20 6. *Load measurement.*

The device as described in connection with figure 3B allows the clinician to detect and record the loads experienced across a joint, and also the load applied across the joint by the device.

25 The motive forces applied across the joints may be from normal physiological loads of the musculoskeletal system or from an externally applied source such as described with reference to figure 4.

It will be noted that the preferred design of the devices described above
30 enable the link assemblies and fixation assemblies to be readily disconnected

from the bone pins 30 in order to replace or adjust the devices during a treatment schedule. Still further, in the preferred designs, the link assemblies may be adjusted in situ. Preferably, the devices will be able to be removed in their entirety within an outpatient clinic.

5

The articulated joint controlling devices of the present invention can be used in the treatment not only of rheumatoid arthritis, but for the treatment of many other conditions such as articular fractures, and following surgical procedures such as osteochondral transfers and joint surface replacement with cartilage graft.

10

Other embodiments are within the scope of the appended claims.

CLAIMS

1. An apparatus for controlling the load on articular cartilage of a human or animal joint comprising:
 - 5 a first fixation assembly for attachment to a first bone;
 - a second fixation assembly for attachment to a second bone; and
 - a link assembly coupled to the first fixation assembly by a first pivot and coupled to the second fixation assembly by a second pivot,
 - the first and second fixation assembly thereby each being angularly
 - 10 displaceable relative to the link assembly.
2. The apparatus according to claim 1 in which the first fixation assembly includes at least one pin for engaging with a first bone.
- 15 3. The apparatus according to claim 2 in which the first fixation assembly includes a clamp for mounting a plurality of pins each for engaging with a first bone, said plurality of pins being spaced along the length of the first fixation assembly.
- 20 4. The apparatus of claim 1 in which the first fixation assembly includes engagement means for engaging at least one bone pin, the engagement means being rotatable about a longitudinal axis of the first fixation assembly.
- 25 5. The apparatus of claim 1 in which the first fixation assembly includes engagement means for engaging at least one bone pin, the engagement means being rotatable about a transverse axis of the first fixation assembly.
6. The apparatus of claim 1 in which the first fixation assembly includes
- 30 engagement means for engaging at least one bone pin, the engagement

means being independently rotatable about a longitudinal axis and a transverse axis of the first fixation assembly

7. The apparatus according to any preceding claim in which the first
5 fixation assembly is coupled to the link assembly by way of a first pivot having one degree of rotational freedom.

8. The apparatus according to any one of claims 1 to 6 in which the first
10 fixation assembly is coupled to the link assembly by way of a first pivot having two degrees of rotational freedom.

9. The apparatus according to any preceding claim in which the link
assembly includes a fixed separation member for maintaining said first and
15 second pivots at a fixed distance of separation.

10. The apparatus according to any preceding claim in which the link
assembly includes a variable separation member for permitting the first and
20 second pivots to vary in their distance of separation within predetermined limits.

11. The apparatus according to claim 10 in which the variable separation
member includes bias means for biasing the first and second pivots towards
a maximum limit of separation distance.

25 12. The apparatus according to claim 10 in which the variable separation
member includes bias means for biasing the first and second pivots towards
a minimum limit of separation distance.

13. The apparatus according to claim 10 in which the variable separation member includes bias means for biasing the first and second pivots towards an intermediate distance of separation between said predetermined limits.
- 5 14. The apparatus according to any preceding claim further including means for limiting the angular displacement of the first fixation assembly relative to the link assembly and/or means for limiting the angular displacement of the second fixation assembly relative to the link assembly.
- 10 15. The apparatus according to any preceding claim further including means for varying separation of the first fixation assembly and the second fixation assembly as a function of the angular displacement of either fixation assembly relative to the link assembly.
- 15 16. The apparatus according to any preceding claim further including a drive member coupled to the first fixation assembly and to the second fixation assembly for controllably varying the angular displacement of the first and second fixation assemblies relative to one another.
- 20 17. The apparatus according to claim 10 in which the variable separation member further includes drive means for controllably varying the distance of separation of the first and second pivots.
18. The apparatus according to any preceding claim further including a
25 sensor adapted to monitor the load applied across the link assembly.
19. The apparatus according to claim 18 in which the sensor is adapted to monitor any one of the tensile load, compression load, shear forces or bending forces applied across the link assembly.

30

20. The apparatus according to claim 19 in which the sensor comprises a strain gauge.
21. The apparatus according to any one of claims 1 to 8 comprising a pair
5 of link assemblies each pivotally anchored to both the first and second fixation assemblies 11, 12 and laterally displaced from one another.
22. The apparatus according to claim 21 in which the pair of link assemblies comprise a first link member and a second link member that are
10 laterally and angularly displaced from one another.
23. The apparatus according to claim 22 in which the first link member and the second link members are disposed in a crosswise formation.
- 15 24. The apparatus according to claim 1 further including a second corresponding apparatus for coupling thereto by a plurality of bone pins.
25. Apparatus substantially as described herein with reference to the accompanying drawings.
- 20 26. A method of controlling loading on a joint comprising the steps of:
attaching a first fixation assembly to a first bone;
attaching a second fixation assembly to a second bone, the second bone being connected to the second bone by an articulating joint;
25 coupling said first fixation assembly and said second fixation assembly by way of a link assembly so that said first fixation assembly and said second fixation assembly are each angularly displaceable relative to the link assembly.

27. The method according to claim 26 further comprising attaching one or both of said fixation assemblies to their respective bones such that the respective bone is rotatable about a longitudinal axis of the fixation assembly.

5

28. The method according to claim 26 further comprising attaching one or both of said fixation assemblies to their respective bones such that the respective bone is rotatable about a transverse axis of the fixation assembly.

10 29. The method according to claim 26 in which the angular displacement permitted between the first fixation assembly and the link assembly and/or between the second fixation assembly and the link assembly respectively comprise one degree of rotational freedom.

15 30. The method according to claim 26 in which the angular displacement permitted between the first fixation assembly and the link assembly and/or between the second fixation assembly and the link assembly respectively comprise two degrees of rotational freedom.

20 31. The method according to any one of claims 26 to 30 further including the step of adjusting a distance of separation of said first and second fixation assemblies to adjust the loading on the joint.

25 32. The method according to any one of claims 26 to 31 further comprising the step of limiting the permitted angular displacement of the first fixation assembly relative to the link assembly and/or limiting the angular displacement of the second fixation assembly relative to the link assembly.

33. The method according to any one of claims 26 to 32 further including the step of varying the angular displacement of the first and second fixation assemblies relative to one another by a powered mechanical drive mechanism.

5

34. The method according to any one of claims 26 to 33 further including the step of deploying a sensor to record load applied across the link assembly.


ABSTRACT

BONE FIXATED, ARTICULATED JOINT LOAD CONTROL DEVICE

5


A load control device can be attached to bones on either side of an articulated joint in order to control the forces and loads experienced by the joint. The device comprises an apparatus for controlling the load on articular cartilage of a human or animal joint and includes: a first fixation
10 assembly for attachment to a first bone; a second fixation assembly for attachment to a second bone; a link assembly coupled to the first fixation assembly by a first pivot and coupled to the second fixation assembly by a second pivot, the first and second fixation assembly thereby each being angularly displaceable relative to the link assembly. The apparatus enables a
15 clinician to effectively control the environment of cartilage in a joint during a treatment episode.

Figure 1

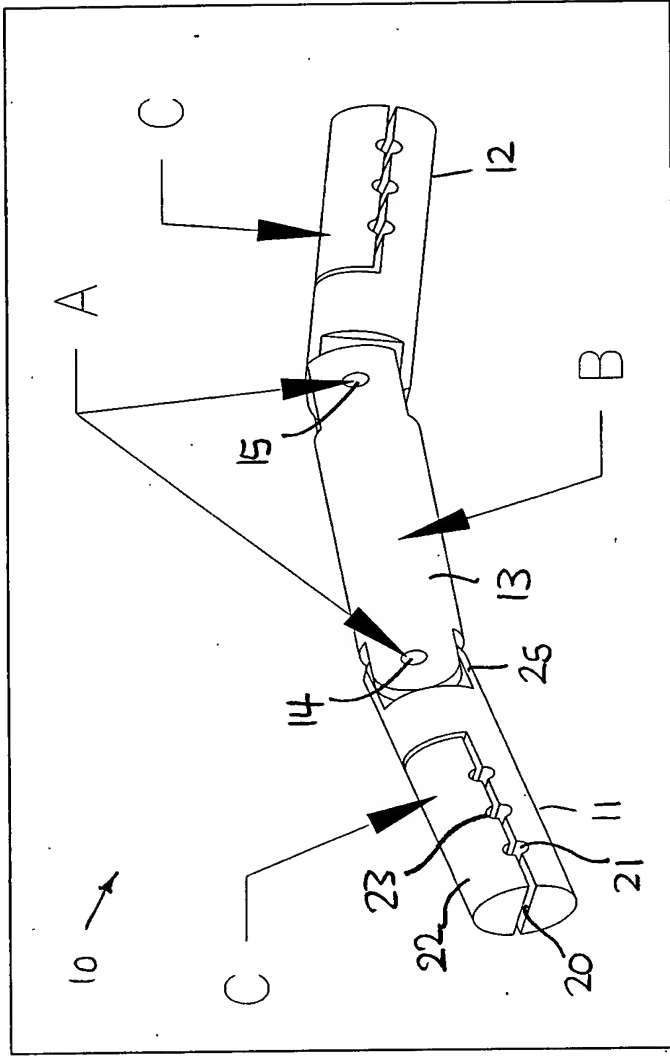


Drawing 1 Preferred embodiment of the device

FIG. 1

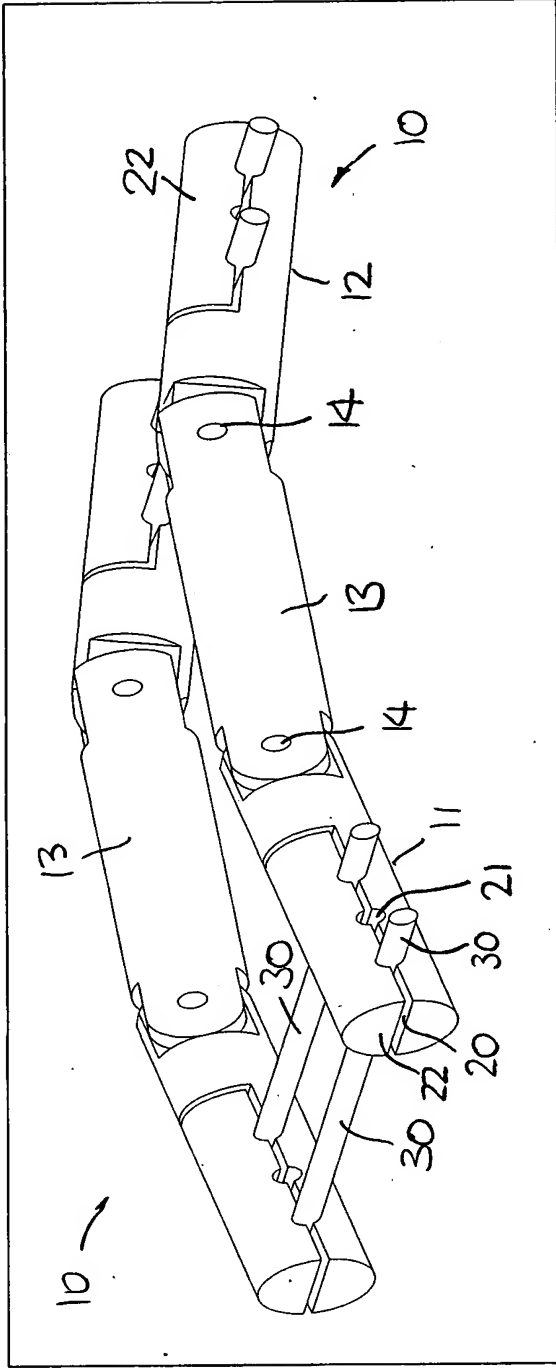


Drawing 2 Device used on both sides of the joint simultaneously

FIG. 2

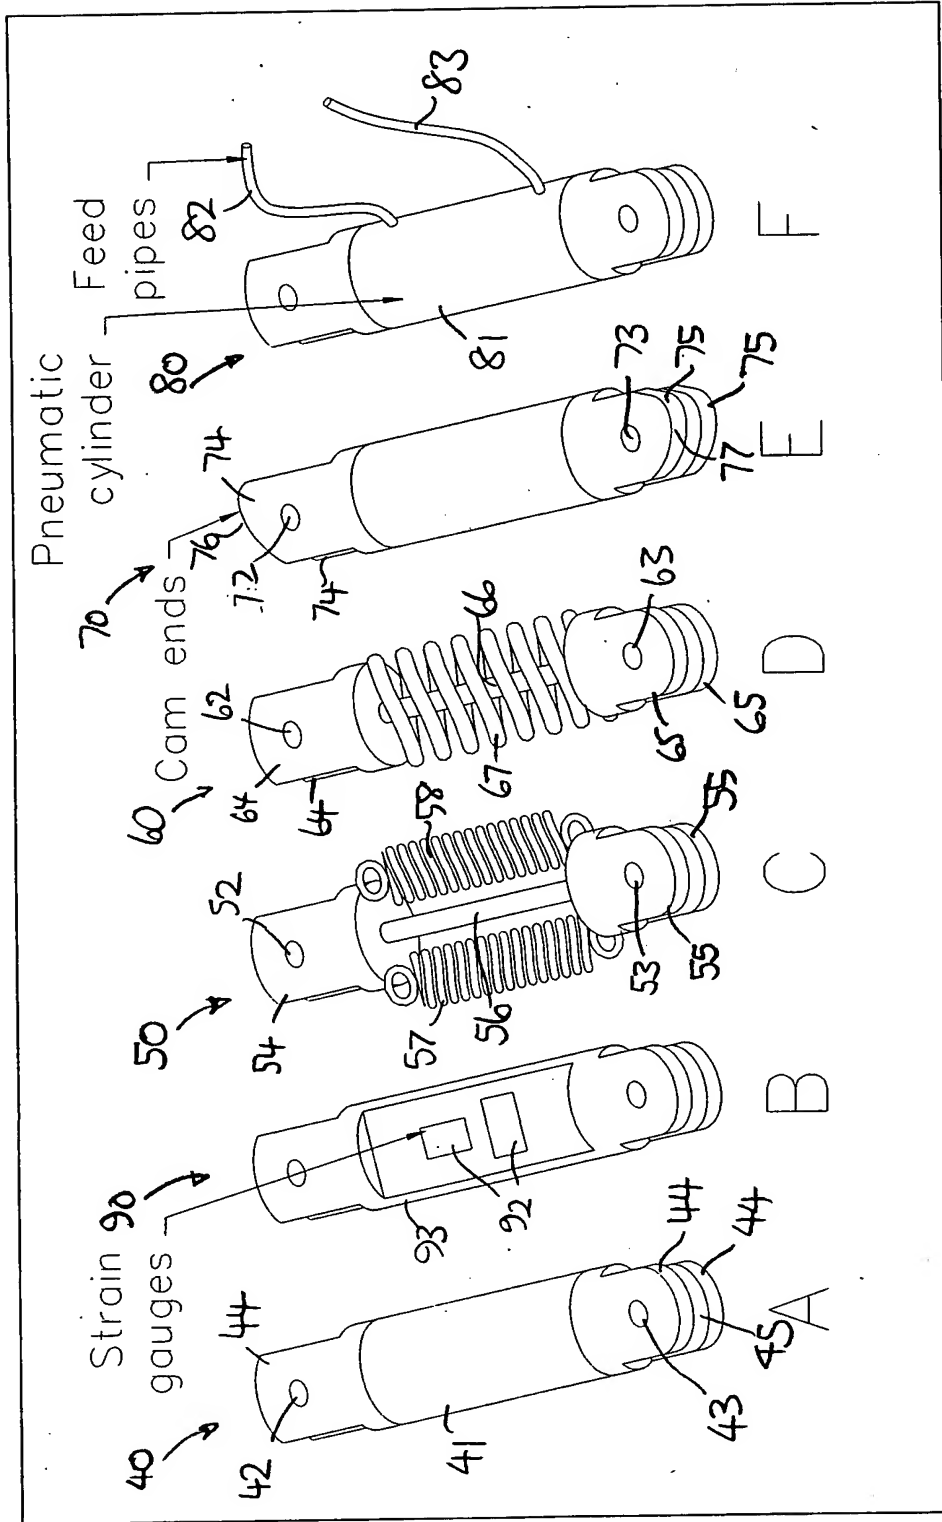

Drawing 3 Various designs of removable central module

FIG. 3

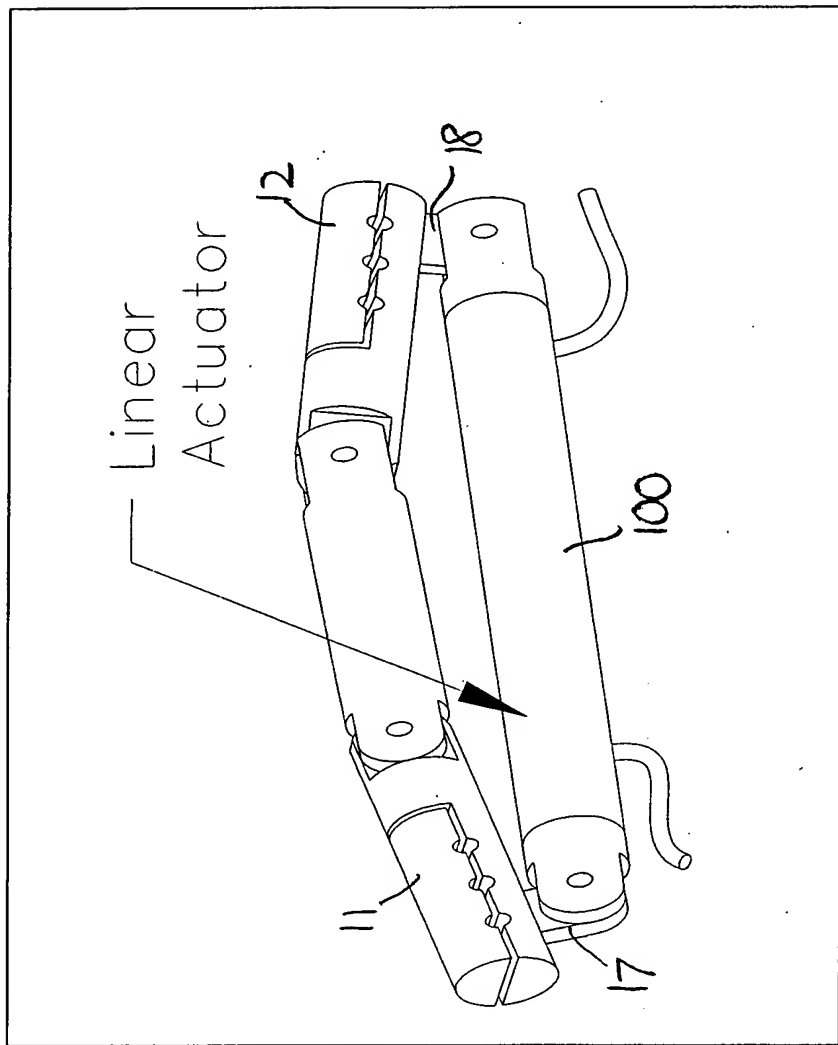

Drawing 4 Externally powered unit to move joint without muscle action

FIG. 4


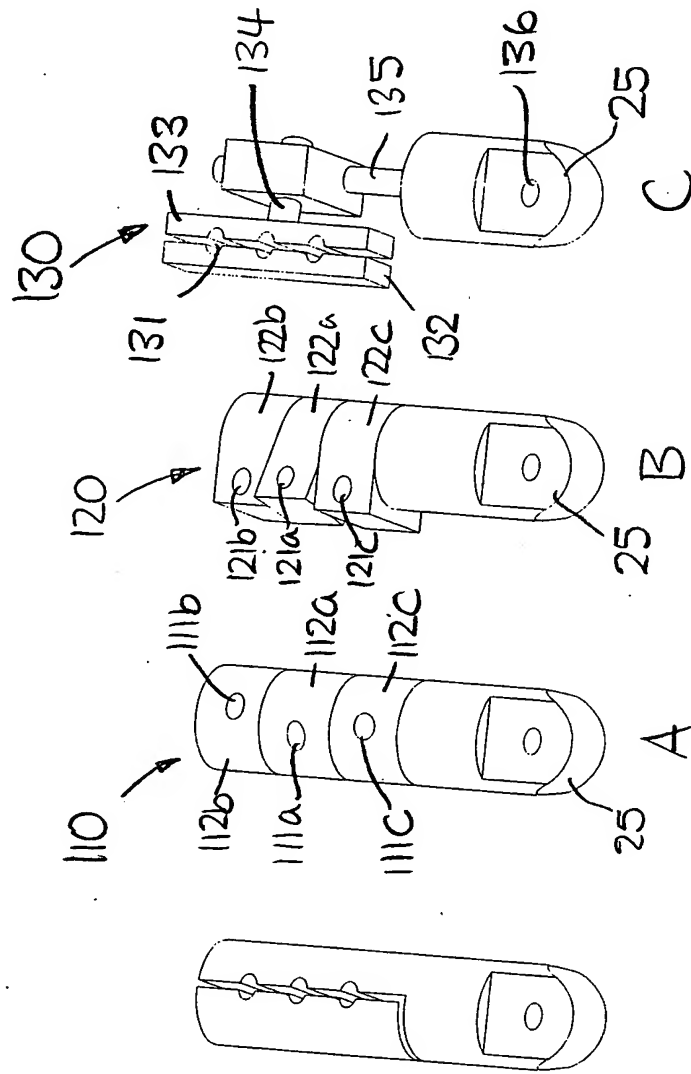


Figure 5

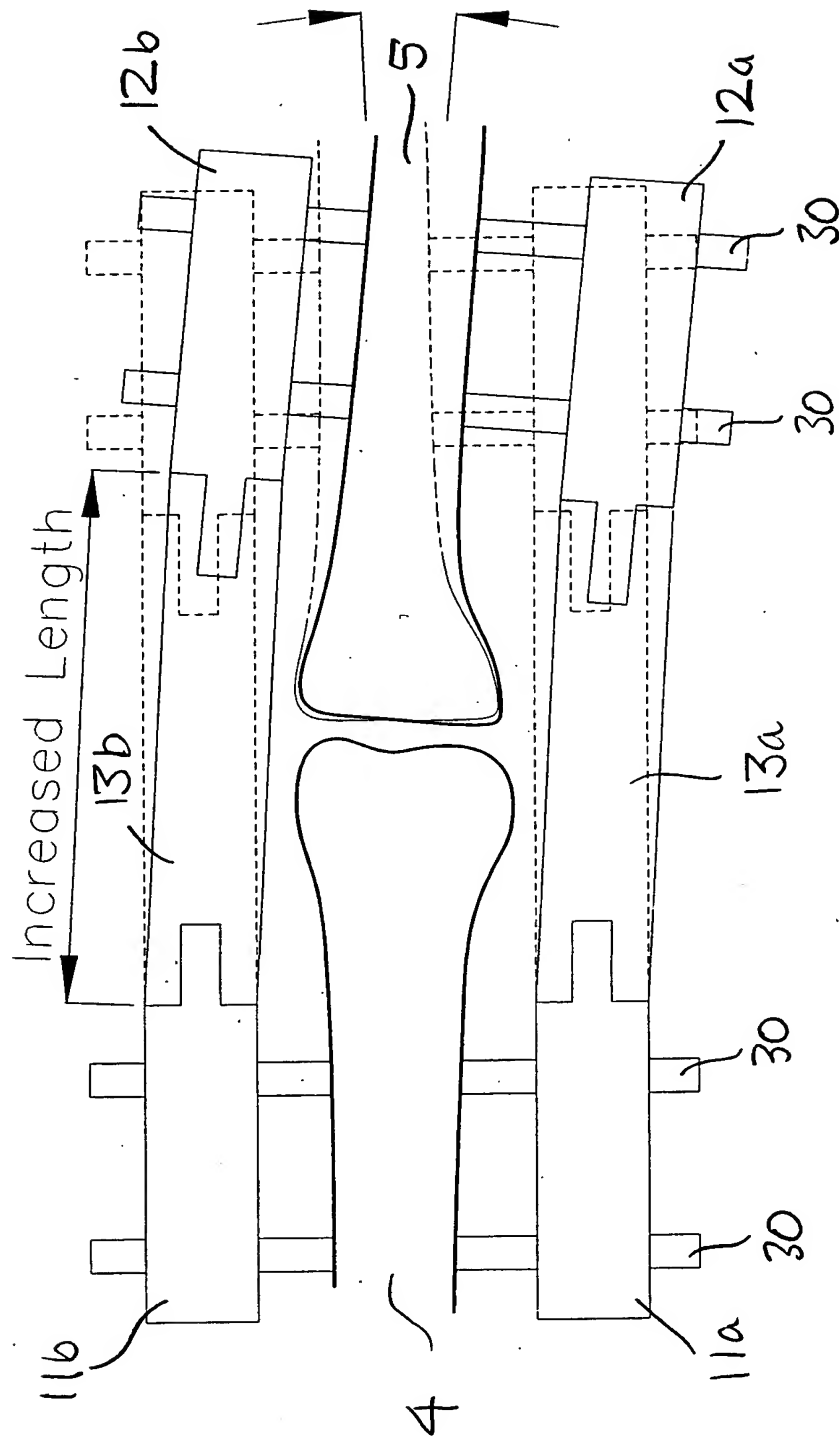

H.G. e.

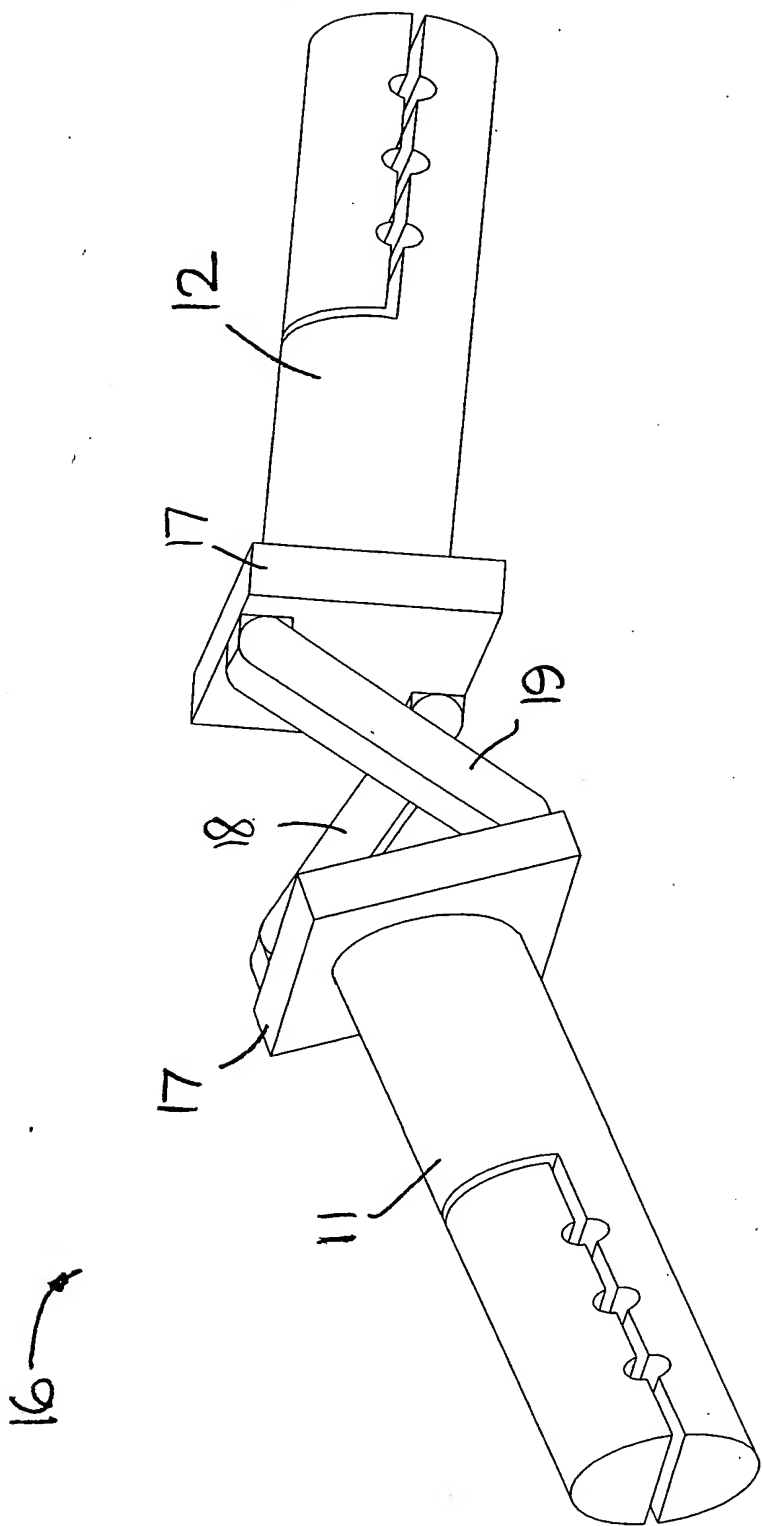


FIG. 7